

This Page Is Inserted by IFW Operations  
and is not a part of the Official Record

## **BEST AVAILABLE IMAGES**

Defective images within this document are accurate representations of the original documents submitted by the applicant.

Defects in the images may include (but are not limited to):

- BLACK BORDERS
- TEXT CUT OFF AT TOP, BOTTOM OR SIDES
- FADED TEXT
- ILLEGIBLE TEXT
- SKEWED/SLANTED IMAGES
- COLORED PHOTOS
- BLACK OR VERY BLACK AND WHITE DARK PHOTOS
- GRAY SCALE DOCUMENTS

**IMAGES ARE BEST AVAILABLE COPY.**

**As rescanning documents *will not* correct images,  
please do not report the images to the  
Image Problem Mailbox.**

# PCT

WORLD INTELLECTUAL PROPERTY ORGANIZATION  
International Bureau



## INTERNATIONAL APPLICATION PUBLISHED UNDER THE PATENT COOPERATION TREATY (PCT)

(51) International Patent Classification 6 : **A61B 5/00, 5/05**  
(11) International Publication Number: **WO 99/39627**  
(43) International Publication Date: **12 August 1999 (12.08.99)**

(21) International Application Number: **PCT/US98/02037**  
(22) International Filing Date: **4 February 1998 (04.02.98)**  
(71) Applicant (for all designated States except US): **DERMAL THERAPY (BARBADOS) INC. (BB/BDI); 261 Bush Hill, Bay Street, Bridgetown (BB).**  
(72) Inventors; and  
(75) Inventors/Applicants (for US only): **ELDEN, Harry, Richardson (US/US); 5500 S.W. 81 Terrace, Miami, FL 33143 (US); WICKETT, R., Randall (US/US); 8351 Jakara Drive, Cincinnati, OH 45255 (US); OLLMAR, Sig (SE/SE); Champijonvagen 51, S-141 60 Huddinge (SE).**

Published  
With international search report.

(74) Agent: **MILLER, Charles E.; Pennie & Edmonds LLP, 1155 Avenue of the Americas, New York, NY 10036-2711 (US).**

(54) Title: **METHOD AND APPARATUS FOR NON-INVASIVE DETERMINATION OF GLUCOSE IN BODY FLUIDS**

(57) Abstract

Method and apparatus for non-invasively determining glucose level in fluid of subject, typically blood glucose level. Impedance of skin tissue is measured and the measurement is used with impedance measurements previously correlated with directly determined glucose levels to determine the glucose level from the newly measured impedance. It is thus possible, to routinely non-invasively determine fluid glucose levels.

### FOR THE PURPOSES OF INFORMATION ONLY

Codes used to identify States party to the PCT on the front pages of pamphlets publishing international applications under the PCT.

AL	Albania	ES	Spain	LS	Lesotho	SI	Slovenia
AM	Armenia	FI	Finland	LT	Lithuania	SK	Slovakia
AT	Austria	FR	France	LU	Luxembourg	SN	Senegal
AU	Australia	GB	Great Britain	LV	Latvia	SZ	Swaziland
AZ	Azerbaijan	GA	Gabon	MC	Monaco	TD	Chad
BA	Bosnia and Herzegovina	GE	Georgia	MD	Moldova	TG	Togo
BB	Barbados	GR	Greece	NE	Niger	TJ	Tajikistan
BE	Belgium	GU	Guam	NG	Nigeria	TM	Turkmenistan
BF	Burkina Faso	HN	Honduras	NO	Norway	TR	Turkey
BG	Bulgaria	IE	Ireland	PL	Poland	TT	Trinidad and Tobago
BJ	Benin	IL	Israel	PT	Portugal	UA	Ukraine
BR	Brazil	IS	Iceland	RO	Romania	UG	Uganda
BY	Belarus	IT	Italy	RU	Russian Federation	US	United States of America
CA	Canada	JP	Japan	SD	Sudan	UZ	Uzbekistan
CF	Congo	KR	Republic of Korea	SE	Sweden	VN	Viet Nam
CG	Congo	KZ	Kazakhstan	SG	Singapore	YU	Yugoslavia
CH	Switzerland	KG	Kyrgyzstan			ZW	Zimbabwe
CI	Cote d'Ivoire	KP	Democratic People's Republic of Korea				
CN	China	LA	Laos				
CU	Cuba	LC	Trinidad and Tobago				
CZ	Czech Republic	LK	Sri Lanka				
DE	Germany	LI	Liechtenstein				
DK	Denmark	LR	Liberia				
EE	Estonia						

## METHOD AND APPARATUS FOR NON-INVASIVE DETERMINATION OF GLUCOSE IN BODY FLUIDS

### FIELD OF THE INVENTION

The present invention relates to non-invasive methods and  
5 devices for determining the level of glucose in a body fluid of a subject.

### BACKGROUND OF THE INVENTION

There are numerous reasons for determining the level of glucose  
present in body fluid of a subject. In the case of a person suffering from  
diabetes, it is often necessary to determine the glucose level in blood daily, or  
10 even more frequently. Non-invasive approaches to determination of blood  
glucose levels have been suggested in the patent literature. For example,  
United States Patent No. 5,036,861 (issued to Sembrowich *et al.* on August 6,  
1991) describes a wrist-mountable device having an electrode which measures  
glucose present in sweat at the skin surface. United States Patent No.  
15 5,222,496 (issued to Clarke *et al.* on June 29, 1993) describes an infrared  
glucose sensor mountable, for instance, on a wrist or finger. United States  
Patent No. 5,433,197 (issued to Stark on July 18, 1995) describes  
determination of blood glucose through illuminating a patient's eye with near-  
infrared radiation. United States Patent Nos. 5,115,133, 5,146,091 and  
20 5,197,951 (issued to Knudson on May 19, 1992, September 8, 1992 and  
January 19, 1993, respectively) describe measuring blood glucose within  
blood vessels of a tympanic membrane in a human ear through light  
absorption measurements. The specifications of all of these patents are  
incorporated herein by reference.

25 The most common current approaches to determining blood  
glucose levels still appear to involve obtaining a sample of the person's blood  
and then measuring the level of glucose in the sample. These approaches will  
not be reviewed here except to say that obtaining the blood sample  
necessarily involves an invasive technique. Generally, the person's skin is  
30 broken or lanced to cause an external flow of blood which is collected in some  
fashion for the glucose level determination. This can be both inconvenient and

- 2 -

distressful for a person and it is an object of the present invention to avoid the  
step of obtaining a blood sample directly, at least on a routine or daily basis.

It is known that skin tissue, when immersed in an aqueous  
glucose solution, equilibrates linearly with the concentration of external  
5 glucose ("Glucose entry into the human epidermis. I. The Concentration of  
Glucose in the Human Epidermis", K.M. Halprin, A. Ohkawara and K. Adachi,  
*J. Invest. Dermatol.*, 49(6): 559, 1967; "Glucose entry into the human  
epidermis. II. The penetration of glucose into the human epidermis *in vitro*",  
K.M. Halprin and A. Ohkawara, *J. Invest. Derm.*, 49(6): 561, 1967). It has also  
10 been shown that skin glucose can vary in synchrony with blood level glucose  
during standardized tolerance testing *in vivo* ("The cutaneous glucose  
tolerance test I. A rate constant formula for glucose disappearance from the  
skin", R.M. Fusaro, J.A. Johnson and J.V. Pilsum, *J. Invest. Dermatol.*, 42:  
359, 1964; "The cutaneous glucose tolerance test", R.M. Fusaro and J.A.  
15 Johnson, *J. Invest. Dermatol.*, 44: 230, 1965). It is also known for  
equilibration of glucose levels to occur between blood and interstitial fluids in  
contact with blood vessels ("A microdialysis method allowing characterization  
of intercellular water space in human", P. Lonnroth, P.-A. Jansson and U.  
Smith, *The American Journal of Physiology*, 253 (Endocrinol. Metab., 16):  
20 E228-E231, 1987; "Assessment of subcutaneous glucose concentration;  
validation of the wick technique as a reference for implanted electrochemical  
sensors in normal and diabetic dogs," U. Fischer, R. Ertle, P. Abel, K. Rebrin,  
E. Brunstein, H. Hahn von Dorsche and E.J. Freyse, *Diabetologia*, 30: 940,  
1987). Implantation of dialysis needles equipped with glucose sensors has  
25 shown that orally ingested glucose load is reflected by parallel changes in skin  
tissue glucose.  
Radio frequency spectroscopy using spectral analysis for *in vitro*  
or *in vivo* environments is disclosed in WO 9739341 (published October 23,  
1997) and WO 9504496 (published February 16, 1995). Measurement of a  
30 target chemical such as blood glucose is described.

- 3 -

# SUMMARY OF THE INVENTION

The present invention is a method and apparatus for non-invasively monitoring levels of glucose in a body fluid of a subject. Typically, blood glucose levels are determined in a human subject.

5 In a preferred embodiment, the invention is a method for non-invasively monitoring glucose in a body fluid of a subject in which the method includes steps of measuring impedance between two electrodes in conductive contact with a skin surface of the subject and determining the amount of glucose in the body fluid based upon the measured impedance. Typically, the body fluid in which it is desired to know the level of glucose is blood. In this way, the method can be used to assist in determining levels of insulin administration.

The step of determining the amount of glucose can include comparing the measured impedance with a predetermined relationship between impedance and blood glucose level, further details of which are described below in connection with preferred embodiments.

In a particular embodiment, the step of determining the blood glucose level of a subject includes ascertaining the sum of a fraction of the magnitude of the measured impedance and a fraction of the phase of the measured impedance. The amount of blood glucose, in one embodiment, is determined according to the equation: Predicted glucose =  $(0.31) \text{ Magnitude} + (0.24) \text{ Phase}$  where the impedance is measured at 20 kHz.

In certain embodiments, impedance is measured at a plurality of frequencies, and the method includes determining the ratio of one or more pairs of measurements and determining the amount of glucose in the body fluid includes comparing the determined ratio(s) with corresponding predetermined ratio(s), i.e., that have been previously correlated with directly measured glucose levels.

In certain embodiments, the method of the invention includes measuring impedance at two frequencies and determining the amount of glucose further includes determining a predetermined index, the index

- 4 -

including a ratio of first and second numbers obtained from first and second of the impedance measurements. The first and second numbers can include a component of said first and second impedance measurements, respectively. The first number can be the real part of the complex electrical impedance at

5 the first frequency and the second number can be the magnitude of the complex electrical impedance at the second frequency. The first number can be the imaginary part of the complex electrical impedance at the first frequency and the second number can be the magnitude of the complex electrical impedance at the second frequency. The first number can be the magnitude of the complex electrical impedance at the first frequency and the second number can be the magnitude of the complex electrical impedance at the second frequency. In another embodiment, determining the amount of glucose further includes determining a predetermined index in which the index includes a difference between first and second numbers obtained from first and second of

15 said impedance measurements. The first number can be the phase angle of the complex electrical impedance at the first frequency and said second number can be the phase angle of the complex electrical impedance at the second frequency.

The skin site can be located on the volar forearm, down to the wrist, or it can be behind an ear of a human subject. Typically, the skin surface is treated with a saline solution prior to the measuring step. An electrically conductive gel can be applied to the skin to enhance the conductive contact of the electrodes with the skin surface during the measuring step.

25 The electrodes can be in operative connection with a computer chip programmed to determine the amount of glucose in the body fluid based upon the measured impedance. There can be an indicator operatively connected to the computer chip for indication of the determined amount of glucose to the subject. The indicator can provide a visual display to the subject.

30

- 5 -

In certain embodiments, the computer chip is operatively connected to an insulin pump and the computer chip is programmed to adjust the amount of insulin flow via the pump to the subject in response to the determined amount of glucose.

5 Electrodes of a probe of the invention can be spaced between about 0.2 mm and about 2 cm from each other.

In another aspect, the invention is an apparatus for non-invasive monitoring of glucose in a body fluid of a subject. The apparatus includes means for measuring impedance of skin tissue in response to a voltage

10 applied thereto and a microprocessor operatively connected to the means for measuring impedance, for determining the amount of glucose in the body fluid based upon the impedance measurement(s). The means for measuring impedance of skin tissue can include a pair of spaced apart electrodes for electrically conductive contact with a skin surface. The microprocessor can be

15 programmed to compare the measured impedance with a predetermined correlation between impedance and blood glucose level. The apparatus can include means for measuring impedance at a plurality frequencies of the applied voltage and the programme can include means for determining the ratio of one or more pairs of the impedance measurements and means for

20 comparing the determined ratio(s) with corresponding predetermined ratio(s) to determine the amount of glucose in the body fluid.

The apparatus preferably includes an indicator operatively connected to the microprocessor for indication of the determined amount of glucose. The indicator can provide a visual display for the subject to read the

25 determined amount of glucose. It is possible that the indicator would indicate if the glucose level is outside of an acceptable range.

In a particular embodiment, the microprocessor is operatively connected to an insulin pump and the apparatus includes means to adjust the amount of insulin flow via the pump to the subject in response to the

30 determined amount of glucose.

- 6 -

The apparatus can include a case having means for mounting the apparatus on the forearm of a human subject with the electrodes in electrically conductive contact with a skin surface of the subject.

In a particular embodiment, the apparatus includes means for

5 calibrating the apparatus against a directly measured glucose level of a said subject. The apparatus can thus include means for inputting the value of the directly measured glucose level in conjunction with impedance measured about the same time, for use by the programme to determine the blood glucose level of that subject at a later time based solely on subsequent impedance

10 measurements.

A microprocessor of the apparatus can be programmed to determine the glucose level of a subject based on the sum of a fraction of the magnitude of the measured impedance and a fraction of the phase of the measured impedance. In a particular embodiment, the apparatus is set to

15 measure impedance at 20 kHz and the microprocessor is programmed to determine the glucose level of a subject based on the equation: Predicted glucose = (0.31)Magnitude + (0.24) Phase.

## BRIEF DESCRIPTION OF THE DRAWINGS

Preferred embodiments of the invention will now be described, reference being had to the accompanying drawings, wherein:

Figure 1 shows plots of various indices as a function of time and glucose concentration based on impedance measurements taken on the skin (SCIM) of a first diabetic subject. Figure 1(a) shows MIX versus measurement number, the timing of the measurements being given in Table 1. Figure 1(b)

25 shows PIX versus measurement number. Figure 1(c) shows RIX versus measurement number. Figure 1(d) shows IMIX versus measurement number. The determinations of MIX, PIX, RIX and IMIX are described in the text.

Figures 2(a), 2(b), 2(c) and 2(d) are similar to Figures 1(a) to 1(d), respectively, but are based on impedance measurement taken on the

30 skin of a second diabetic subject.

- 7 -

Figure 3 is a plot showing the reading (average of ten readings) of a dermal phase meter as a function of directly determined blood glucose concentration. Measurements were taken on a site on the left forearm (+) and right forearm (-); and

5 Figure 4 is similar to Figure 3, but readings were taken at a finger.

#### DETAILED DESCRIPTION OF PREFERRED EMBODIMENTS

A preferred method of the invention involves directly contacting a subject's skin with an electrode, taking one or more impedance measurements and determining the subject's blood glucose level based on the impedance measurement(s). Preferably, there is a computer programmed to make the determination based on the impedance measurement(s). In one aspect, the invention includes deriving a number of indices from one or more measurements of impedance between poles of the electrode. The value(s) of the one or more indices is an indicator of, i.e. correlates with, the subject's blood glucose level.

Thus, the invention is illustrated below by laboratory feasibility tests to establish that a correlation between one or more such index values based on impedance measurement(s) and a subject's blood glucose level exists. The tests were conducted using particular parameters, for example impedance measurements obtained at a certain frequency or certain frequencies, and particular indices were derived therefrom. It will be understood that other and/or additional frequencies may be found to be more optimal and that other indices may well be found to be more optimal.

#### 25 Examples

Each of two subjects was treated as indicated in Table 1.

Impedance measurements were taken at the volar forearm using the "SCIM" apparatus described below. Impedance measurements were taken at thirty-one frequencies and four different indices were determined using two of the

- 8 -

frequencies: 20 and 500 kHz. Directly measured blood glucose levels of each subject are indicated in Table 1.

Table 1: Treatment Regimen of Subjects				
5	Measurement No. - time (minutes)		Blood Glucose Measurement First Subject	Blood Glucose Measurement Second Subject
	0	0	154	141
10	Ingest 50 g glucose			
	1	10	146	164
	2	20	174	194
	3	30	246	232
	4	40	228	257
15	Ingest 50 g glucose			
	5	50	268	304
	6	60	255	348
	7	70	320	346
	8	80	320	355
20	9	90	399	361
	10	100	343	383
	11	110	334	381
	Rapid insulin administered		4 units	8 units
	12	125	358	379
25	13	140	377	346
	14	155	353	333

Four indices, MIX, PIX, RIX and IMIX were determined (see below) and plotted as a function of time. Results are shown in Figures 1 and

- 9 -

2, the data collected prior to the first glucose ingestion being assigned "0" on the x-axis of each plot.

Spearman rank order correlation coefficients were determined, and are presented Table 2 and 3 for the first and second subjects, respectively. A value of  $P < 0.05$  is often considered to be a satisfactory correlation. As can be seen in Table 2, a satisfactory correlation was obtained for both the MIX and the IMIX indices for the first subject. As can be seen in Table 3, a satisfactory correlation was obtained for the MIX, PIX and IMIX indices for the second subject. The value of P for the RIX index was very

close to being satisfactory. It must be borne in mind that these values were obtained from a small sample set and yet a clear indication of a satisfactory correlation for more than one index has been obtained in these experiments. Optimization of the parameters of frequency and the choice of index or indices might well lead to a significant improvement on the results given here.

15

**Table 2: Statistical Analysis of Relationship between Measured Glucose Levels and Selected Indices for First Subject**

Pair of Variables	Spearman Rank Order Correlations		
	Valid N	Spearman R	P
Glucose Level & MIX	15	-.722719	-3.77028
Glucose Level & PIX	15	.865832	6.23942
Glucose Level & RIX	15	-.418980	-1.66372
Glucose Level & IMIX	15	-.710833	-3.64385
			0.002972

20

- 10 -

**Table 3: Statistical Analysis of Relationship between Measured Glucose Levels and Selected Indices for Second Subject**

Pair of Variables	Spearman Rank Order Correlations		
	Valid N	Spearman R	P
Glucose Level & MIX	15	-.616622	-2.82405
Glucose Level & PIX	15	.266547	.99712
Glucose Level & RIX	15	-.477094	-1.95731
Glucose Level & IMIX	15	-.607686	-2.75888
			0.016260

5

10 The impedance measurements on which the results shown in Figures 1 and 2 are based were obtained using a Surface Characterizing Impedance Monitor (SCIM) developed by Ollmar (United States Patent No. 5,353,802, issued October 11, 1994; "Instrument evaluation of skin irritation", P.Y. Rizvi, B.M. Morrison, Jr., M.J. Grove and G.L. Grove, *Cosmetics & Toiletries*, 111: 39, 1996; "Electrical impedance index in human skin: Measurements after occlusion, in 5 anatomical regions and in mild irritant contact dermatitis", L. Emtestam and S. Ollmar, *Cont. Derm.* 28: 337, 1975; "Electrical impedance for estimation of irritation in oral mucosa and skin", S. Ollmar, E. Eek, F. Sundstrom and L. Emtestam, *Medical Progress Through Technology*, 21: 29, 1995; "Electrical impedance compared with other non-invasive bioengineering techniques and visual scoring for detection of irritation in human skin", S. Ollmar, M. Nyren, I. Nicander and L. Emtestam, *Brit. J. Dermatol.* 130: 29, 1994; "Correlation of impedance response patterns to histological findings in irritant skin reactions induced by various surfactants", I. Nicander, S. Ollmar, A. Eek, B. Lundh Rozell and L. Emtestam, *Brit. J. Dermatol.* 134: 221, 1996) which measures bioelectrical impedance of the skin at multiple frequencies. The instrument is basically an AC-bridge fabricated from standard laboratory instruments: a function generator, a digital oscilloscope, impedance references, and a driver for the probe.

15 The indices plotted in Figures 1 and 2 were determined as follows:

20 The indices plotted in Figures 1 and 2 were determined as follows:

25 The indices plotted in Figures 1 and 2 were determined as follows:

30

- $MIX \text{ (magnitude index)} = \text{abs}(Z_{20kHz}) / \text{abs}(Z_{500kHz})$   
 $PIX \text{ (phase index)} = \arg(Z_{20kHz}) - \arg(Z_{500kHz})$   
 $RIX \text{ (real part index)} = \text{Re}(Z_{20kHz}) / \text{abs}(Z_{500kHz})$   
 $IMIX \text{ (imaginary part index)} = \text{Im}(Z_{20kHz}) / \text{abs}(Z_{500kHz})$
- 5 where  $\text{abs}(Z_i)$  is the magnitude (modulus) of the complex electrical impedance at the frequency  $i$ ,  $\arg(Z_i)$  the argument (phase angle) in degrees,  $\text{Re}(Z_i)$  the real part of the complex electrical impedance, and  $\text{Im}(Z_i)$  the imaginary part of the complex electrical impedance. The magnitudes and phase angles are delivered by the instrument, and the real and imaginary parts are calculated according to the elementary complex number relationships:  $\text{Re}(Z_i) = \text{abs}(Z_i) \cdot \cos[\arg(Z_i)]$  and  $\text{Im}(Z_i) = \text{abs}(Z_i) \cdot \sin[\arg(Z_i)]$ .

10 The RIX reflects changes mainly in conductivity; the IMIX reflects mainly reactance changes, which are of capacitive nature; the MIX reflects changes along the length of the vector describing the impedance in complex space, which will be emphasized if the real and imaginary parts change in the same direction and proportion; the PIX will be emphasized if the real and imaginary parts change in different directions and/or in different proportions.

Prior to contacting a subject's skin with the electrode, the skin is treated with a 0.9% saline solution by holding a soaked gauze against the measurement site for about a minute and then wiping the site with a dry cloth. The purpose of this step is to ensure adequate electrical coupling between the skin and the probe (electrode) in order to reduce variability that may introduced into the measurements by stratum corneum. A person skilled in the art would understand that variations are possible, and more optimal pre-treatment conditions may be obtainable.

Blood glucose levels were determined directly from a blood sample using a lancet prick and measuring the blood glucose concentration with an Elite Glucometer according to manufacturer's instructions (Elite Glucometer, Miles Canada, Diagnostics Division, Division of Bayer).

30 In a second set of experiments, 31 subjects were tested using the SCIM apparatus. A baseline measurement was taken and standardized food

packet ingested. Two additional impedance measurements were taken one half hour and one hour after the initial measurement and blood glucose levels determined directly. Multiple regression analysis was carried out on data obtained at 20 kHz and relationship (1) established:

5

Predicted glucose = (0.31) Magnitude + (0.24) Phase;  $F=5.5$ ,  $p<0.005$

The multiple R for the prediction was 0.33.

The SCIM instrument was used to measure impedance measured at 31 different frequencies logarithmically distributed in the range of 1 kHz to 1 Mhz (10 frequencies per decade). Subsequent determinations were based, in the first set of experiments, on two of the frequencies: 20 and 500kHz; and in the second set of experiments, 20 kHz only. It may be found in the future that there is a more optimal frequency or frequencies. It is quite possible, in a commercially acceptable instrument that impedance will be determined at at least two frequencies, rather than only one. For practical reasons of instrumentation, the upper frequency at which impedance is measured is likely to be about 500 kHz, but higher frequencies, even as high as 5 MHz or higher are possible and are considered to be within the scope of this invention.

20 Relationships may be established using data obtained at one, two or more frequencies.

It may be found to be preferable to use an artificial neural network to perform a non-linear regression.

25 A preferred instrument, specifically for determining glucose levels of a subject, includes a 2-pole measurement configuration that measures impedance at multiple frequencies, preferably two well spaced apart frequencies. The instrument includes a computer which also calculates the index or indices that correlate with blood glucose levels and determines the glucose levels based on the correlation(s).

30 The invention is also illustrated by experiments that were carried out with a dermal phase meter (DPM) available from Nova™ Technology



- 13 -

Corporation of Gloucester, Massachusetts. Measurements were taken with the dermal phase meter at two skin sites, the forearm and the middle finger. The scale of the meter is from 90 to 999. It is thought that a higher reading indicates a higher degree of skin hydration. Blood glucose measurements were also measured directly (Mgs/dL) using an Elite Glucometer determined directly from a blood sample using a lancet prick and measuring the blood glucose concentration according to manufacturer's instructions (Elite Glucometer, Miles Canada, Diagnostics Division, Division of Bayer). Typical results are shown in Figures 3 and 4. Measurements were taken at various times to track changes in skin hydration from that present while fasting overnight, attending ingestion of a typical meal for breakfast or lunch and following a peak of blood glucose and decline to about 100 Mgs/dL.

In these experiments, a probe sensor was placed against the skin surface and held lightly until the instrument indicated completion of data acquisition. Time interval (latch time) for data acquisition was selected at zero seconds (instantaneous). Other suitable time periods can be anywhere 0 and 30 seconds, or between 0.5 and about 10 seconds, or between about 1 and 5 seconds or about 5 seconds. The results obtained using the dermal phase meter are plotted as function of blood glucose concentration in Figures 3 and 4, respectively. Each plotted point represents the average of 10 measurements using the dermal phase meter. Studies were performed in the morning on fasting subjects. After baseline measurements on fasting, food was ingested to raise blood glucose levels. Studies continued until blood glucose levels declined to baseline levels.

Figures 3 and 4 indicate that the Nova™ meter reading of the skin increases with increasing blood glucose concentration.

In one aspect of the invention, electrodes of a device are placed in conductive contact with a subject's skin in order to measure impedance (Z) at various frequencies (f) in a range from a few Hertz (hz) (say 10 hz) to about 5 Mhz. A more typical range would be between 1 kHz and 1 Mhz, and more likely between 5 kHz and 500 kHz. Electrodes of the device are electrically

- 14 -

connected to a metering device which indicates the impedance at a selected frequency of applied voltage, as understood by a person skilled in the art. In a particular embodiment, the device is programmed to operate at the selected frequencies in rapid sequence. Alternative modes of operation are possible, for example, the voltage can be rapidly increased with time and Fourier transformation carried out to obtain a frequency spectrum. Ratios of impedance measured at various frequencies are determined and the blood glucose level of the subject is measured directly. This process is repeated at different times so as to make the determination at a number of different glucose levels. In this way, ratios of impedance determined at particular frequencies which are found to reproducibly reflect a person's blood glucose levels over a range of glucose levels are determined. The ratios of measured impedance at the selected frequencies can thus be correlated with directly measured glucose levels, that is, a plot in which  $\log(Z_1/Z_2)$  vs  $\log(f)$  is a linear correlation, or an approximately linear correlation, is determined. This relationship is then used to determine the blood glucose level of the person directly from ratios of similarly obtained impedance measurements, thus avoiding an invasive technique for obtaining the blood glucose level. Impedance includes both resistance and reactance.

It may be found for a proportion of the population that there is a universal set of impedance frequency ratios, thus avoiding the necessity of determining individual correlations.

The general approach described for the foregoing aspect of the invention can be used in connection with other indicas based on impedance measurements, such as MIX, PIX, RIX and IMIX described above.

It is important, of course, to be able to reliably reproduce results as much as possible in order for this type of device to be useful. To this end an appropriate skin site is chosen. Generally speaking, an undamaged skin site and one that is not heavily scarred would be chosen. A skin site having a stratum corneum which is less likely to deleteriously interfere with the measurements is chosen. A likely possibility is the volar forearm, down to the

wrist, or behind an ear. The skin surface can be treated just prior to measurement in order to render the stratum corneum more electrically transparent by application, for example, of a physiological saline dressing for about a minute. Excess liquid should be removed before application of the probe.

Given the importance of reliable glucose level determinations in setting insulin administrations, it is important that the invention be used only in circumstances in which it is known that the approach described herein reliably indicates glucose levels of a subject. It is possible that the invention would not be suitable for use with a given proportion of the population or 100% of the time with a given individual. For example, an individual may have a skin condition which deleteriously interferes with impedance measurements, making it difficult to assume that impedance measurements can reliably indicate a person's blood glucose level. For such a person, a different approach to glucose level determination would be more suitable.

An apparatus that utilizes a neural network to carry out analyses based on impedance could be trained for a specific subject, or possibly a group of subjects. An example of such a group of subjects might be subjects of the same sex, belonging to a particular age group and within particular height and weight ranges.

It may be advantageous to optimize the spacing of the electrodes of the probe. That is, it may be found that the electrodes of a SCIM probe are too close to each other to provide maximally reproducible results. An object of a suitable probe is to have electrodes spaced from each other to obtain optimal penetration of current into tissue containing glucose in its interstitial spaces. It is expected that electrodes spaced somewhere between about 0.2 mm and about 2 cm are suitable.

Additionally, the use of a gel can improve skin-probe contact to more reliably produce useful measurements, as would be known to a person skilled in the art, e.g., a gel comprising mostly water in combination with a

thickener such as Cellulose, glycerin or propylene glycol as a moisturizer, and a suitable preservative.

An apparatus for non-invasive monitoring of glucose in a body fluid of a subject includes means for measuring impedance of skin tissue in response to a voltage applied thereto, i.e. a probe. There is a computer processor operatively connected to the means for measuring impedance for determining the blood glucose level based upon one or more impedance measurements. The microprocessor is programmed to calculate the blood glucose level of a subject based upon impedance measurements taken at one or more frequencies. In a particular embodiment, a calculation based upon impedance at a single frequency, along the lines of that shown in relationship (1), is carried out by the processor. In another embodiment, the calculation includes determining MIX and/or IMIX. The calculation might include determining PIX. The calculation might include determining RIX. It might be necessary to calibrate an individual apparatus for use with a particular subject. In such case, the apparatus includes means for calibrating the apparatus against a directly measured glucose level of that subject. The apparatus could thus include means for inputting the value of the directly measured glucose level in conjunction with impedance measured about the same time, for use by the programme to determine the blood glucose level of that subject at a later time based solely on subsequent impedance measurements.

In one embodiment, a meter is worn in which a probe is continuously in contact with the skin and moisture buildup between occlusive electrodes and the skin is sufficient to obtain useful measurements. The device can be mountable on a person's forearm, much like a wristwatch. Such an embodiment might not prove to be useful for all subjects.

As previously stated, it might be found to be necessary for a meter to be calibrated individually, that is, it might be necessary to determine the relationship between ascertained impedance ratios or index or indices of interest, and blood glucose levels of an individual and base the operation of the particular meter for that individual on the relationship. To this end, a

- 17 -

preferred monitoring device of the invention includes means for calibrating the relationship between a directly measured blood glucose level and an index or indices of interest.

Because blood glucose level determinations of the present invention are non-invasive and relatively painless it is possible to make such determinations with a greater frequency than with a conventional pin-prick method. In a particularly advantageous embodiment, blood glucose levels are monitored quite frequently, say every fifteen or five, or even one minute or less, and an insulin pump is interfaced with the meter to provide continual control of blood glucose in response to variations of blood glucose levels ascertained by means of the meter.

The disclosures of all references, and particularly the specifications of all patent documents, referred to herein, are incorporated herein by reference.

The invention now having been described, including the best mode currently known to the inventors, the claims which define the scope of the protection sought for the invention follow.

15

- 18 -

# CLAIMS

1. A method for non-invasively monitoring glucose in a body fluid of a subject, the method comprising:

measuring impedance between two electrodes in conductive contact with a skin surface of the subject; and  
determining the amount of glucose in the body fluid based upon the measured impedance.

5

2. The method of claim 1 wherein the body fluid is blood.

3. The method of claim 2 wherein determining the amount of glucose includes comparing the measured impedance with a predetermined relationship between impedance and blood glucose level.

10

4. The method of claim 1, 2 or 3 wherein the subject is human.

5. The method of claim 1, 2 or 3, including measuring impedance at a plurality of frequencies, determining the ratio of one or more pairs of measurements and wherein determining the amount of glucose in the body fluid includes comparing the determined ratio(s) with corresponding predetermined ratio(s).

15

6. The method of claim 5 wherein the skin surface is located on the volar forearm.

7. The method of claim 6 wherein the skin surface is treated with a saline solution prior to the measuring step.

20

8. The method of claim 7 wherein an electrically conductive gel is applied to the skin to enhance the conductive contact of the electrodes with the skin surface during the measuring step.

9. The method of claim 1, 2 or 3, wherein the electrodes are in operative connection with a computer chip programmed to determine the amount of glucose in the body fluid based upon the measured impedance.

25

10. The method of claim 9 wherein an indicator is operatively connected to the computer chip for indication of the determined amount of glucose to the subject.

11. The method of claim 10 wherein the indicator provides a visual display to the subject.

30

- 19 -

12. The method of claim 9 wherein the computer chip is operatively connected to an insulin pump and the computer chip is further programmed to adjust the amount of insulin flow via the pump to the subject in response to the determined amount of glucose.

13. The method of claim 1, 2 or 3, wherein the electrodes are spaced between about 0.2 mm and about 2 cm from each other.

14. The method of claim 1 wherein determining the amount of glucose includes measuring impedance at two frequencies.

15. The method of claim 14 wherein determining the amount of glucose further includes determining a predetermined index, the index comprising a ratio of first and second numbers obtained from first and second of said impedance measurements.

16. The method of claim 15 wherein each of said first and second numbers includes a component of said first and second impedance measurements, respectively.

17. The method of claim 16 wherein said first number is the real part of the complex electrical impedance at the first frequency and the second number is the magnitude of the complex electrical impedance at the second frequency.

18. The method of claim 16 wherein said first number is the imaginary part of the complex electrical impedance at the first frequency and the second number is magnitude of the complex electrical impedance at the second frequency.

19. The method of claim 16 wherein said first number is the magnitude of the complex electrical impedance at the first frequency and said second number is the magnitude of the complex electrical impedance at the second frequency.

20. The method of claim 14 wherein determining the amount of glucose further includes determining a predetermined index, the index comprising a difference between first and second numbers obtained from first and second of said impedance measurements.

21. The method of claim 20 wherein said first number is the phase angle of the complex electrical impedance at the first frequency and said second

- 20 -

number is the phase angle of the complex electrical impedance at the second frequency.

22. The method of claim 1 or 2 wherein determining the amount of glucose includes ascertaining the sum of a fraction of the magnitude of the measured impedance and a fraction of the phase of the measured impedance.

23. The method of claim 2 including determining the amount of blood glucose according to the equation of relationship (1).

24. An apparatus for non-invasive monitoring of glucose in a body fluid of a subject, the apparatus comprising:

10 means for measuring impedance of skin tissue in response to an voltage applied thereto; and

a microprocessor operatively connected to the means for measuring impedance, for determining the amount of glucose in the body fluid based upon the impedance measurement.

15 25. The apparatus of claim 24, wherein said means for measuring impedance of skin tissue includes a pair of spaced apart electrodes for electrically conductive contact with a skin surface.

26. The apparatus of claim 25, wherein said microprocessor is programmed to compare the measured impedance with a predetermined correlation between impedance and blood glucose level.

27. The apparatus of claim 26, including means for measuring impedance at a plurality frequencies of said applied voltage, wherein the programme further includes means for determining the ratio of one or more pairs of the impedance measurements and means for comparing the determined ratio(s) with corresponding predetermined ratio(s) to determine the amount of glucose in the body fluid.

28. The apparatus of claim 24, 25, 26 or 27, further comprising an indicator operatively connected to the microprocessor for indication of the determined amount of glucose.

29. The apparatus of claim 28 wherein the indicator provides a visual display.

30. The apparatus of claim 28 wherein the microprocessor is operatively connected to an insulin pump and includes means to adjust the amount of insulin flow via the pump to the subject in response to the determined amount of glucose.

31. The apparatus of claim 25, 26 or 27 wherein the electrodes are spaced between about 0.2 mm and about 2 cm from each other.

32. The apparatus of claim 28 including a case having means for mounting the apparatus on the forearm of a human subject with the electrodes in said electrically conductive contact with a skin surface of the subject.


33. The apparatus of claim 24, further comprising:  
means for calibrating the apparatus against a directly measured glucose level of a said subject.

34. The apparatus of claim 25 or claim 33, wherein the microprocessor is programmed to determine the glucose level of a subject based on the sum of a fraction of the magnitude of the measured impedance and a fraction of the phase of the measured impedance.

35. The apparatus of claim 34, wherein the microprocessor is programmed to determine the glucose level of a subject based on the equation of relationship (1).

20

FIG. 1

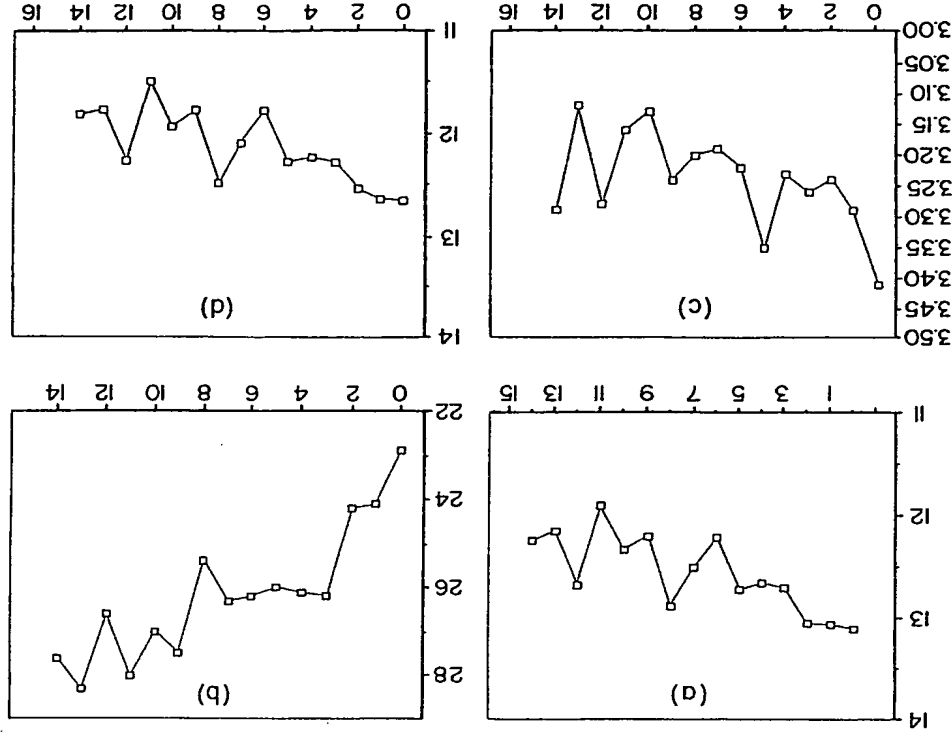

2/3

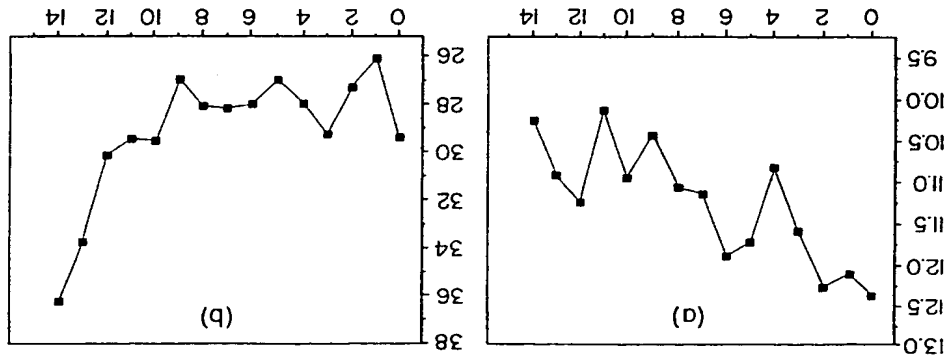


FIG. 2

3/3

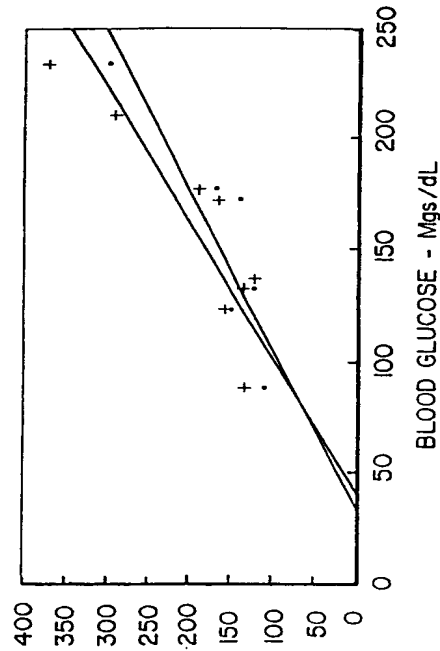


FIG. 3

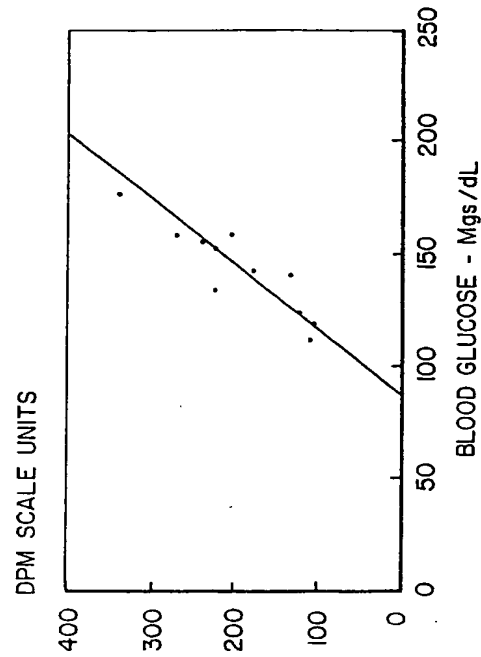


FIG. 4

# INTERNATIONAL SEARCH REPORT

International Application No. <b>PCT/US 98/02037</b>	
A. CLASSIFICATION OF SUBJECT MATTER <b>IPC 6 A61B5/00 A61B5/05</b>	
According to International Patent Classification (IPC) or to both national classification and IPC	
B. FIELDS SEARCHED Minimum documentation searched (classification system followed by classification symbols) <b>IPC 6 A61B 601N</b>	
Documentation searched other than minimum documentation to the extent that such documents are included in the fields searched	
Electronic data base consulted during the international search (name of data base and, where practical, search terms used)	
C. DOCUMENTS CONSIDERED TO BE RELEVANT	
Category	Citation of document, with indication, where appropriate, of the relevant passages
A	WO 93 18402 A (UNIVERSITY COLLEGE OF WALES) ) 16 September 1993 see page 1, line 6 - page 3, line 32 see page 4, line 10 - page 6, line 25 see figures
A	WO 95 04496 A (SOLID STATE FARMS, INC.) 16 February 1995 cited in the application see page 6, line 16 - page 8, line 2 see page 18, line 30 - page 19, line 14 see figure 1 --- -/-
Further documents are listed in the continuation of box C.	
Special categories of cited documents:	
"A" document defining the general state of the art which is not considered to be of particular relevance	"T" later document published after the international filing date or priority date and not in conflict with the applicant's invention
"E" earlier document but published on or after the international filing date	"X" document of particular relevance: the claimed invention cannot be considered novel or cannot be considered to
"L" document which may know details on priority claim(s) or which is cited to establish the publication date of another claim or other special reason (as specified)	"Y" document of particular relevance: the claimed invention cannot be considered to be novel or cannot be considered to be inventive, such combination being obvious to a person skilled in the art.
"O" document referring to an oral disclosure, use, exhibition or other means	"G" document member of the same patent family
"P" document published prior to the international filing date but after the priority date claimed	
Date of the actual completion of the international search	
15 June 1998	Date of mailing of the international search report
Name and mailing address of the ISA European Patent Office, P.O. Box 5618 Postfach 2 NL - 2280 HV Rijswijk Tel. (+31-70) 340-3040, Tx. 31 051 epo nl Fax: (+31-70) 340-3010	
Authorized officer Chen, A	

# INTERNATIONAL SEARCH REPORT

International Application No. <b>PCT/US 98/02037</b>	
C. DOCUMENTS CONSIDERED TO BE RELEVANT	
Category	Citation of document, with indication, where appropriate, of the relevant passages
A	ZAMZOW ET AL.: "Development and evaluation of a wearable blood glucose monitor" ASAIO TRANSACTIONS, vol. 36, no. 3, July 1990, TORONTO, CA, pages 588-591, XP000204509 see page 588, right-hand column, line 1 - see page 591, left-hand column, line 41 see figures 1, 2
A	DE 19 34 139 A (FORSTER) 21 January 1971 see page 3, line 1 - page 8, line 11 see figure 1 --- 1, 24
Further documents are listed in the continuation of box C.	
Special categories of cited documents:	
"A" document defining the general state of the art which is not considered to be of particular relevance	"T" later document published after the international filing date or priority date and not in conflict with the applicant's invention
"E" earlier document but published on or after the international filing date	"X" document of particular relevance: the claimed invention cannot be considered novel or cannot be considered to
"L" document which may know details on priority claim(s) or which is cited to establish the publication date of another claim or other special reason (as specified)	"Y" document of particular relevance: the claimed invention cannot be considered to be novel or cannot be considered to be inventive, such combination being obvious to a person skilled in the art.
"O" document referring to an oral disclosure, use, exhibition or other means	"G" document member of the same patent family
"P" document published prior to the international filing date but after the priority date claimed	
Date of the actual completion of the international search	
Date of mailing of the international search report	
Name and mailing address of the ISA European Patent Office, P.O. Box 5618 Postfach 2 NL - 2280 HV Rijswijk Tel. (+31-70) 340-3040, Tx. 31 051 epo nl Fax: (+31-70) 340-3010	
Authorized officer Chen, A	

# INTERNATIONAL SEARCH REPORT

Information on patent family members

Patent document cited in search report		Publication date		Patent family member(s)		International Application No	
WO 9318402 A		16-09-1993		AU 662400 B CA 2127355 A EP 0629291 A JP 7504579 T NO 943114 A US 5569591 A		PCT/US 98/02037	
WO 9504496 A		16-02-1995		US 5508203 A AU 676082 B AU 7520294 A EP 0714259 A			
DE 1934139 A		21-01-1971		NONE			